


HPLC Report

Structure :SELANK
 Lot NO :P230214-LR271657
 Number :0200049
 Column :250*4.6mm,Kromasil-C18-5um
 Solvent A:0.1%TFA in 100%water
 Solvent B:0.1%TFA in 100%acetonitrile

| Gradient : | A | B |
|------------|------|------|
| 0.1min | 93% | 7% |
| 25.0min | 68% | 32% |
| 25.1min | 0% | 100% |
| 30.0min | stop | |

Flow rate:1.0ml/min
 Wavelength(nm):220
 Volume :10ul

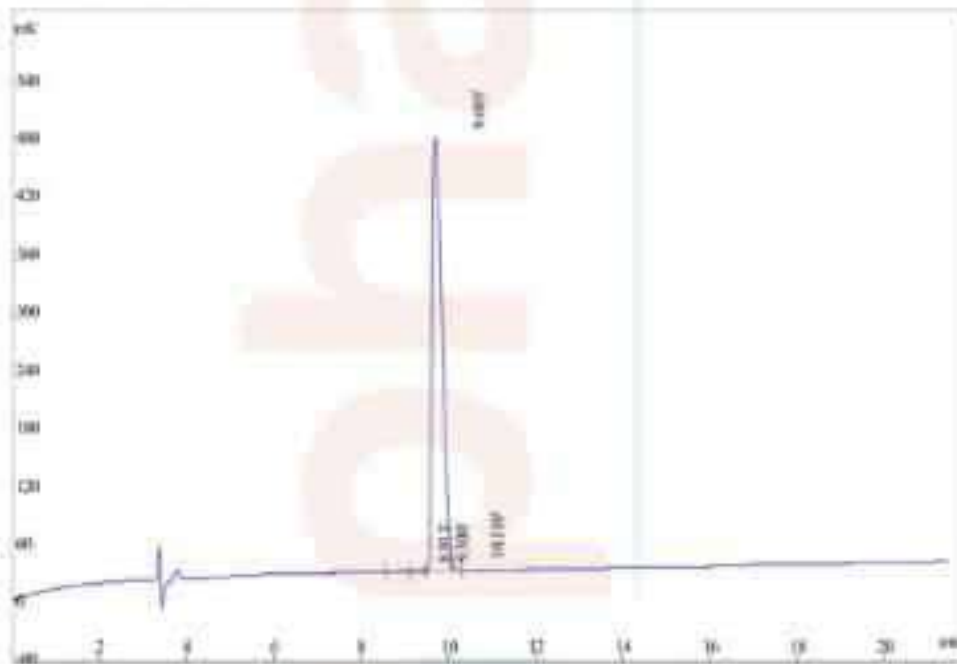


| Rank | Time | Conc. | Area | Height |
|-------|--------|--------|---------|--------|
| 1 | 8.913 | 0.3695 | 25480 | 2466 |
| 2 | 9.300 | 0.2318 | 15985 | 1392 |
| 3 | 9.685 | 98.92 | 6819678 | 449037 |
| 4 | 10.110 | 0.4835 | 33338 | 4189 |
| Total | | 100 | 6894481 | 457084 |

HPLC Report

Structure : SEMAX
 Number : 010250036
 Lot No : P230213-LR486110
 Column : 4.6×250mm,Venusil XBP-C18
 Solvent A : 0.1% trifluoroacetic in 100% acetonitrile
 Solvent B : 0.1% trifluoroacetic in 100% water
 Gradient :

| | A | B |
|---------|------|-----|
| 0.01min | 25% | 75% |
| 25min | 50% | 50% |
| 25.1min | 100% | 0% |
| 30min | STOP | |

Flow rate : 1.0 mL/min
 Wavelength : 220nm
 Volume : 5ul

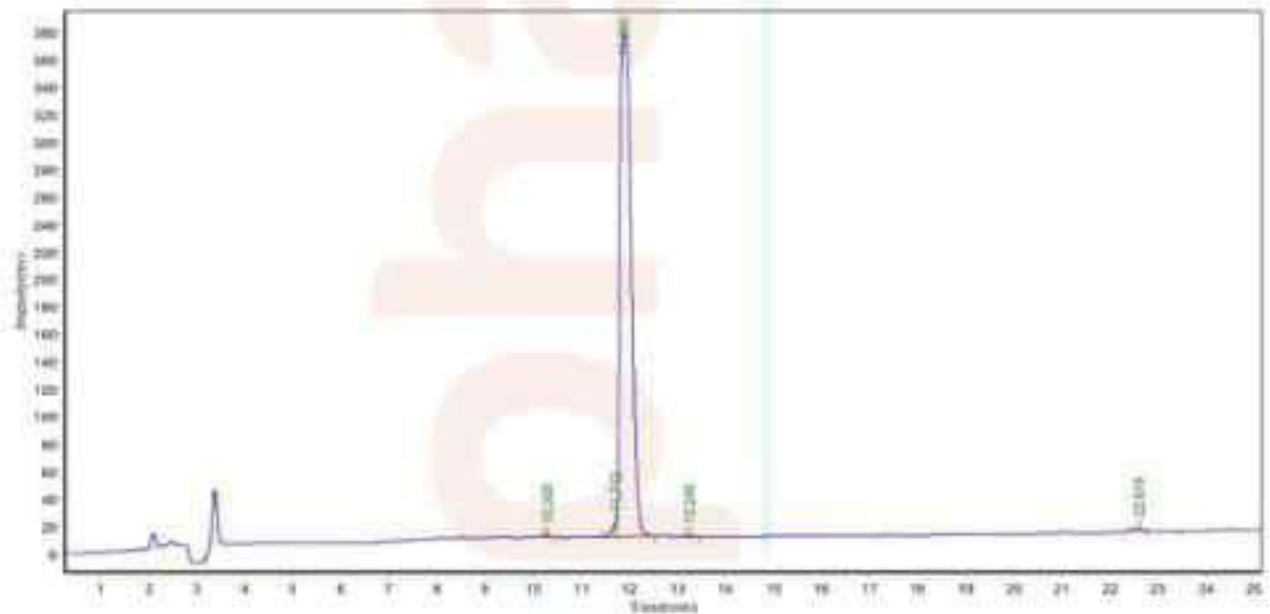

| Peak No. | Ret Time | Height | Area | Conc. |
|--------------|----------|------------|-------------|-----------------|
| 1 | 10.300 | 920.250 | 7080.791 | 0.1193 |
| 2 | 11.712 | 9360.205 | 41465.055 | 0.6984 |
| 3 | 11.900 | 364530.438 | 5868836.500 | 98.8538 |
| 4 | 13.245 | 505.647 | 4207.098 | 0.0709 |
| 5 | 22.618 | 1145.281 | 15293.985 | 0.2576 |
| Total | | | | 100.0000 |